

# From Sample To Patient Chart 4 To 8 Times Faster.

**Gram-Negative I.D.'s in 4 hours. Nonfermenter I.D.'s in as little as 6 hours. Yeasts in less than 24 hours. Gram-Negative Susceptibilities in 4 to 10 hours. Gram-Positive I.D.'s in 4 to 12 hours, Susceptibilities in 6 to 10.**



Test times of the Vitek System are 4 to 8 times faster than manual or semi-automated techniques. They are not mere incremental improvements, but dramatic changes which have revolutionized the role of microbiology, worldwide. Yesterday, microbiology played a purely confirmatory role. With today's Vitek, it can be a diagnostic tool as well.

Until now, anti-microbial therapy was often begun without definitive bacterial identification. With the Vitek, accurate medication begins hours (sometimes *days*) earlier than any other system or technique allows.

Prove to yourself that the Vitek System is more vital to you than ever in an atmosphere of cost-containment. Put us to the test. Challenge us to demonstrate the value of our System in our literature and, ultimately, in *your* lab with *your* workload.

Just mail the coupon, below. Or call.

## PUT US TO THE TEST.

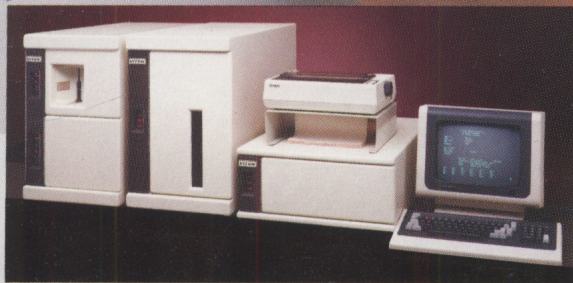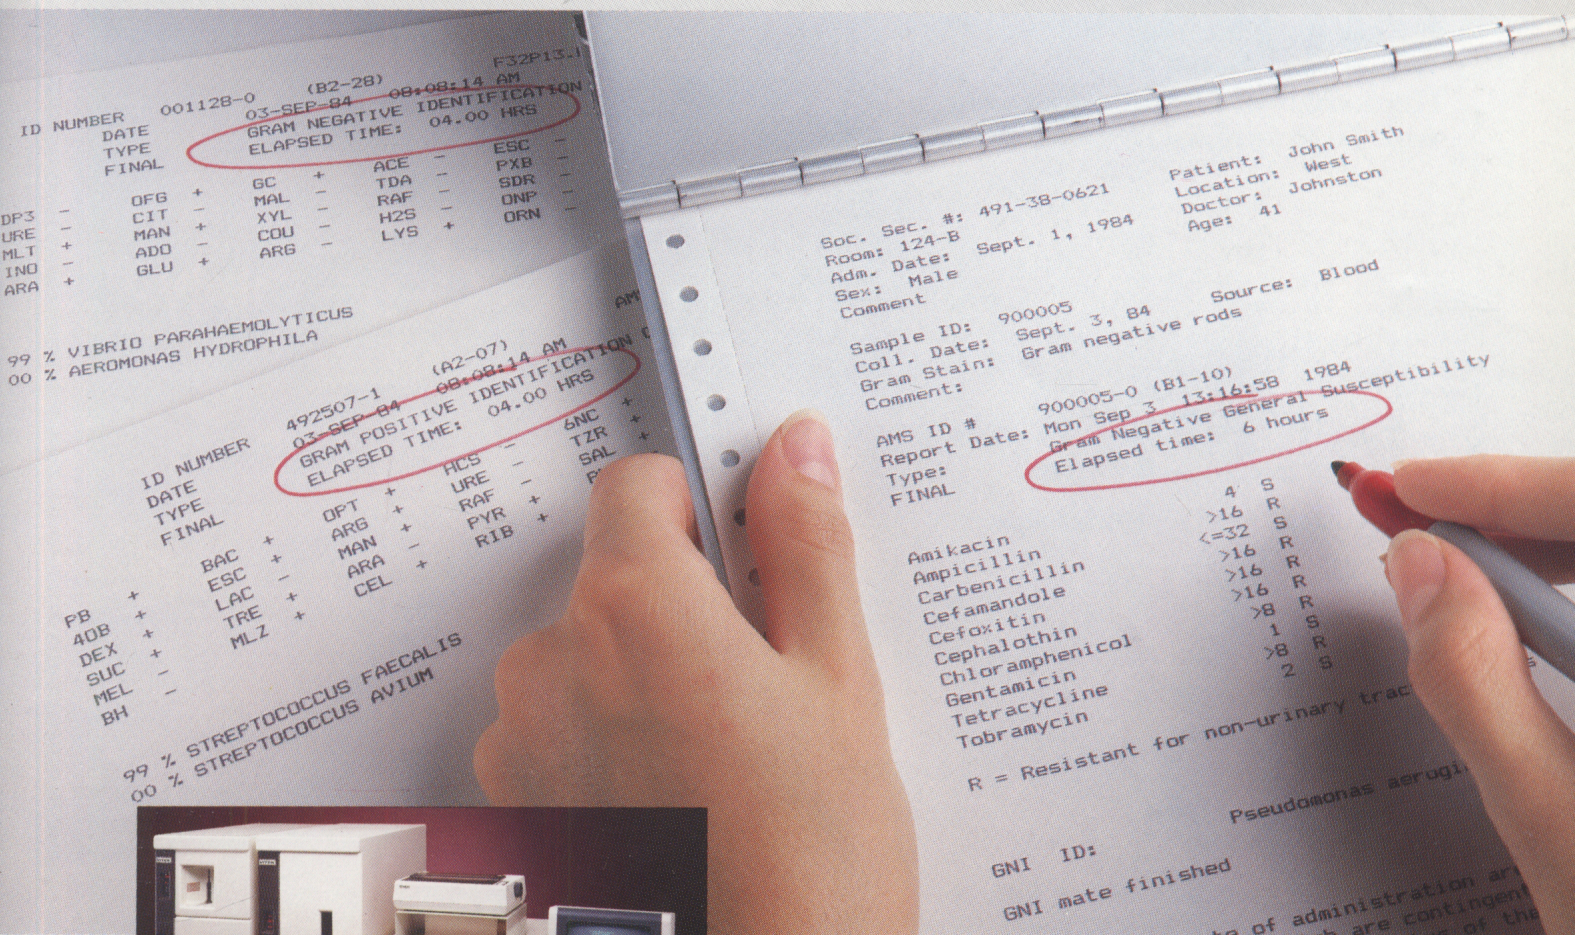

# VITEK

A SUBSIDIARY OF  
MCDONNELL DOUGLAS CORPORATION

595 Anglum Drive • Hazelwood, MO 63042 USA  
800-325-1977 • In Missouri, 314-232-0887

<https://doi.org/10.1017/S0195941700060628> Published online by Cambridge University Press

### I'd Like To Put The Vitek System To The Test.

- Please send your brochure.
- Have a salesperson phone me.

Name \_\_\_\_\_

Title \_\_\_\_\_ Phone \_\_\_\_\_  
(Area Code)

Hospital \_\_\_\_\_

Address \_\_\_\_\_

City \_\_\_\_\_ State \_\_\_\_\_ Zip \_\_\_\_\_


**New CIDEX\*  
Products for Hemodialysis**

The most trusted name in disinfection...

# Now for your dialysis unit's special needs

## CIDEX\*

Hemodialysis Disinfection System with Dialyzer Disinfecting Solution

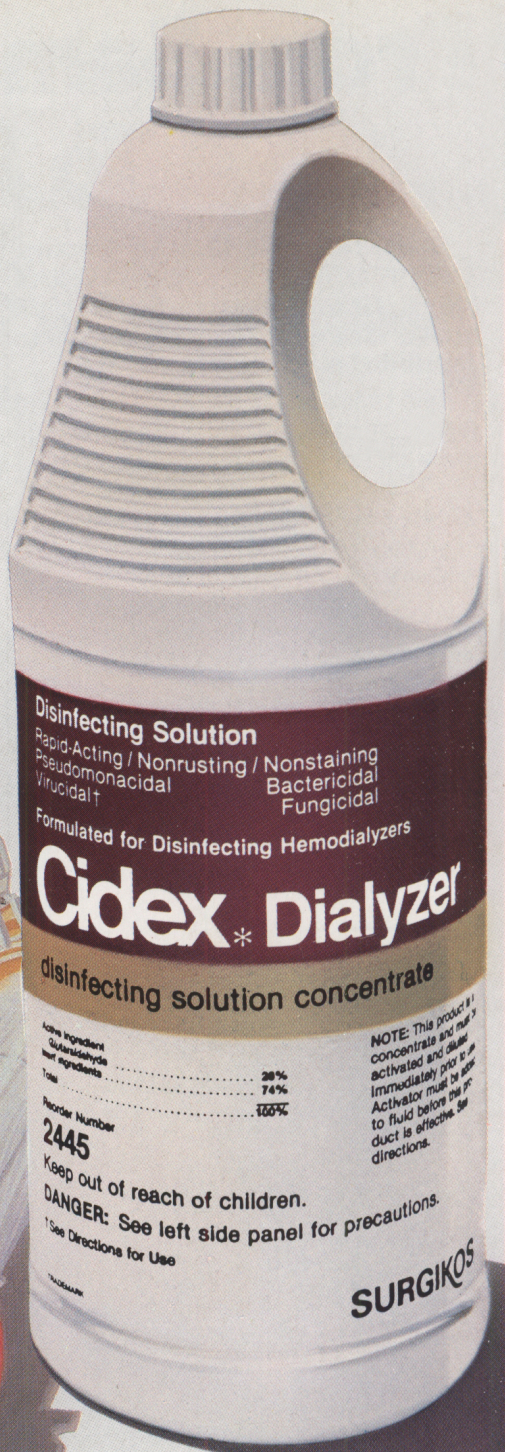

### CIDEX Dialyzer Disinfecting Solution

- Clinically tested—safe, nonmutagenic, effective
- No formaldehyde odor
- Lower active ingredient level—requires less rinsing time than formaldehyde
- Residual Test Kit detects one part per million active ingredient—faster and far more sensitive than formaldehyde residual tests
- For use in all current reprocessing systems
- Proven efficacy against viruses, bacteria and pathogenic fungi

**All of these advantages—plus cost efficiency when compared to other disinfection systems.**

### CIDEX HD Disinfecting Solution

- Proven effective
- Recommended by leading equipment manufacturers
- Complemented by an Effectiveness Test Kit and a Residual Test Kit.

For more information write: CIDEX Product Director, SURGIKOS, P.O. Box 130, Arlington, Texas 76010

**Disinfecting Solution**  
Rapid-Acting / Nonrusting / Nonstaining  
Pseudomonacidal / Bactericidal  
Virucidal / Fungicidal

Formulated for Disinfecting Hemodialyzers

**Cidex\* Dialyzer**  
disinfecting solution concentrate

Active ingredient	
Gutachloride	28%
Water	72%
Total	100%

Product Number  
**2445**

Keep out of reach of children.  
**DANGER: See left side panel for precautions.**  
\* See Directions for Use

**SURGIKOS**

**SURGIKOS**  
a Johnson & Johnson company

SURGIKOS, INC., ARLINGTON, TEXAS 76010

\*Trademark © SURGIKOS 1984 S-4024

<http://doi.org/10.1017/S019541100160128> Published online by Cambridge University Press