

Liquid Nitrogen Safety

Charles J. Butterick,

Texas Tech University Health Sciences Center

Recent Internet postings on the Microscopy listserv indicate paradoxical views on the personal protective equipment (PPE) necessary to handle liquid nitrogen (LN2) safely. Those views range from full protective gear to, somewhat facetiously, complete nudity. The crux of the paradox is that both extremes have points of validity.

The gist of preventing frostbite or cold injury to the skin is to prevent continuous contact with LN2. The physics of the Leidenfrost effect (LE) protects the skin from momentary contact or splashes of LN2. A layer of gas between the LN2 and the skin prevents significant heat transfer from the skin, stopping damage. The LE does not apply to inadvertent splashes of LN2 to the cornea. Alternatively, using protective equipment insulates the skin and prevents trapping of the cryogen by allowing the LN2 to run off.

Safety information and diagrams from Reichert-Jung cryopreparation instrumentation manuals demonstrate the non-trapping concept well. Other cryogen safety recommendations can be found in the CRC Handbook of Laboratory Safety, 3rd edition, pages 315-317 and Handbook of Compressed Gases, 3rd edition, pages 75-79. A local cryogen supplier should also be able to provide safety information. The following is a synthesis of safety recommendations for the use of LN2.

Full face shields or safety glasses with side guards work well to protect the eyes. Safety goggles or glasses that allows LN2 to be trapped against the face or eyes are not recommended.


Since TEM users with EDXA systems have to lift a dewar to head level or higher, a full face shield, long sleeve shirt buttoned close to the neck, and cryogen gloves with tight wrists, or loose gloves with a cuff, extending over the wrist of the sleeve is recommended. LN2 will not be able to dribble or splash from the dewar and become trapped between the shirt and skin. Partially unbuttoned shirts or low-cut blouses should be avoided. Other users can wear short sleeve shirts. Long cuffless trousers should extend over the shoes or boots. Individuals wearing pants tucked into boots, skirts, shorts, or sweats with elastic at the ankle may create a situation where LN2 can run down the leg or splash into the shoe, become trapped between the shoe and foot, resulting in injury. Those wearing shorts, skirt or sweats are safer working with LN2 wearing sandals with no heel strap or socks. Wearing sandals, though common and accepted in parts of academia, is an unsafe practice in a laboratory environment.

If one is merely pouring LN2 from one large dewar into a smaller container, gloves are not suggested so long as all jewelry, watches and bracelets are removed from hands and arms. Cold metal objects are safely handled with a moderately thick potholder. If gloves are used, the fit should be loose so that they may be shed quickly in the event of a spill. Some cryogen gloves have a much tighter fit but also have elastic on the cuff to prevent LN2 from rolling into the glove and becoming trapped against the skin. Latex, or similar, gloves should not be used while working with LN2. The latex can freeze rapidly, hold the intense cold against the skin and cause injury.

One liter of LN2 generates approximately 700 liters of gaseous nitrogen at room temperature. Adequate ventilation is necessary because nitrogen is tasteless and odorless. A spill of 3 L of LN2 in an 8 m³ (5 X 8 X 9 ft.) elevator causes the oxygen level to decrease from a normal 21% to 17%, a dangerously low level with various physiological effects (12% oxygen causes unconsciousness). The great volume expansion of LN2 as it warms is the reason any transfer container must allow the constant release of gaseous nitrogen.

Use of LN2 in a wide mouth container without a cover, if undisturbed for a time, causes differential distillation of pure gas layers over the cryogen. Sparking the oxygen layer in the presence of organic materials or flammables can cause a flash explosion. Such LN2 containers should be kept loosely covered as much as possible and away from any flammables.

An individual dressed minimally to safely handle LN2 (in accordance with the LE) would not be safely dressed for other hazards in the lab. Clothing and footwear appropriate for the lab dictate the use of personal protective equipment to shed any spilled or splashed LN2. While this recommendation will not be welcomed by all, an appropriate safety procedure predicts areas of hazard - and leads even experienced individuals away from the slightest possibility of accident or injury. ■

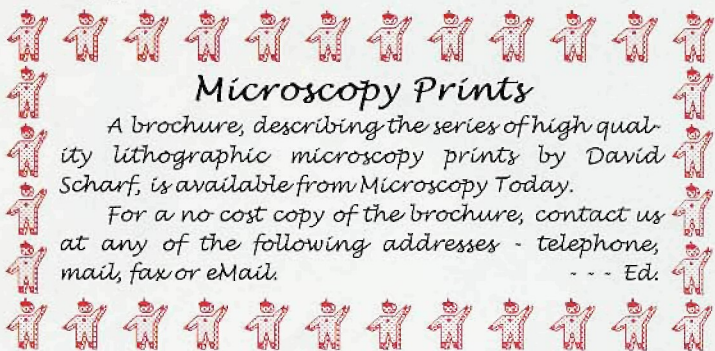

Microscopy Prints

A brochure, describing the series of high quality lithographic microscopy prints by David Scharf, is available from Microscopy Today.

For a no cost copy of the brochure, contact us at any of the following addresses - telephone, mail, fax or eMail.

- - - Ed.

Front Page Image

SEM Photograph of a Chigger Mite (Trombicula Alfreddugesi)

Imaged on an ETEC SEM at 5 kV using the SEM Wideband Multi-Detector Color Synthesizer (designed, built and patented by David Scharf). Then acquired digitally at 2,048 X 1,536 pixels directly into a Macintosh Power PC as a TIFF file, using Digital Micrograph software and Digiscan hardware. Then output to a CELCO film recorder, using Ektachrome 100+ film, to produce a 4x5 transparency.

Photograph is Copyright© by David Scharf, 1994
All Rights Reserved.

This image is available at 1,000X as a 18 1/2" x 19" high quality, lithographic print from Microscopy Today.

MICROSCOPY TODAY

A monthly newsletter dedicated to the unique interests in microscopy of, and mailed at no cost to, some 8,000 microscopists worldwide.

PO Box 620122, Middleton, WI 53562 - Tel.: (608)836-1970 - Fax: (608)836-1969 - eMail: MicroToday@aol.com

Copyright in 1996 by Today Enterprises. All rights reserved.

Don Grimes, Editor

Launch Your Field Emission SEM Capabilities To The 4nm At 1kV Level.

The Amray Model 3600 LEAP

(Low Energy Advanced Performance) can propel your field emission SEM performance beyond current boundaries to a new standard of excellence. The Amray 3600 LEAP delivers:

- high resolution – 4nm at 1kV, 1.5nm at 15kV
- optimized geometry for a short working distance at high tilts with large samples (6mm w.d. at 45° tilt)
- high kV (25kV) for uncompromised analytical capabilities
- highly reliable patented Schottky field emission gun
- 2048 x 2048 frame buffer for advanced digital imaging
- two 17" high resolution, 1000 line viewing monitors
- 5 axes motorized eucentric stage
- motorized 8" linear load lock for rapid sample exchange
- embedded computer control for all SEM functions

The Amray 3600 LEAP provides resolution that's out of this world – call 1-800-225-1462 for complete information on the Model 3600 LEAP and other Amray systems.



AMRAY

160 Middlesex Tpke., Bedford, MA 01730 Tel: 617-275-1400 Fax: 617-275-0740

Circle Reader Inquiry #12