

Full-field X-ray Nano-scope Developed at SSRF

Biao Deng¹, Yudan¹ Wang, Yuqi Ren¹, Tianxi Sun², Guangzhao¹ Zhou, Guohao Du¹, Fen Tao¹, Honglan Xie¹, Tiqiao Xiao¹

¹. Shanghai Institute of Applied Physics, CAS, Shanghai, China

². Beijing Normal University, Beijing, China

Full-field X-ray nano-scope is one of the most powerful tools for in-situ, non-destructive observation of the inner structure of objects with high resolution. Many X-ray nano-scope systems have been constructed in the world and have realized 30nm spatial resolution with 20 microns field of view(FOV). Based on the user operation experiences of years at Shanghai Synchrotron Radiation Facility(SSRF) X-ray imaging beamline, we get to know that lots of user experiments will rely on X-ray full-field nano-CT with big FOV and 100nm scale resolution. A full-field X-ray nano-imaging system has been designed and constructed at SSRF [1]. The microscope is based on a beam shaper and a zone plate using both absorption contrast and Zernike phase contrast, with the optimized energy set to 10keV. The experimental test results by a Siemens star pattern demonstrate that a spatial resolution of 100 nm is achieved, while an FOV of 50 μm is obtained [2]. And a full-field X-ray nano-CT system based Equally Sloped Tomography(EST) was developed. 3D imaging of tantalum particles reconstructed by EST with 128 projections was reported [3]. The nano-scope is ready to be opened to users. And a dedicated full field X-ray nano-imaging beamline based on bending magnet is under construction in the SSRF phase-II project. The beamline aims at the 3D imaging of the nano-scale inner structures. The photon energy range is of 5-14keV. The design goals with the FOV of 20 microns and a spatial resolution of 20nm are proposed at 8 keV.

In full-field X-ray nano-imaging, the most commonly used condenser devices are zone plates and ellipsoidal moncapillaries. In contrast, the transmission efficiency of ellipsoidal glass moncapillary is higher than that of zone plates. Therefore, ellipsoidal moncapillaries are generally adopted as focusing lenses in full-field transmission X-ray nano-imaging. An ellipsoidal glass moncapillary was designed and fabricated and its performance was measured by both optical measurement and synchrotron radiation X-ray test. The moncapillary had slope errors as low as 15 μrad rms. The images of the focal spot and the far-field pattern recorded by X-ray detector showed that the focusing size was 40 μm and divergences was 1.86mrad at 9keV. Based the moncapillary, a full Field Transmission X-ray Microscopes(TXM) System was designed and constructed at SSRF. The spatial resolution of 100 nm was achieved by utilizing the moncapillary condenser [4,5], which indicating the ellipsoidal moncapillary had high quality and could meet the requirement of X-ray nano-imaging. In the future, a new moncapillary will be fabricated for and used as condenser in SSRF TXM beamline for 20nm TXM.

References:

- [1] Biao Deng et al. SPIE, **8851** (2013), p. 88511D-1
- [2] Binggang Feng et al. CHINESE OPTICS LETTERS **14** (2016), p. 093401.
- [3] Yudan Wang, Yuqi Ren, Guangzhao Zhou, et al, (submitted)
- [4] Fen Tao, Yudan Wang, Yuqi Ren, et al. ACTA OPTIC SINICA **37** (2017), p. 0034002.
- [5] Bowen Jiang, Zhiluo Liu, Xuepeng Sun, et al. Optics Communications **398** (2017), p. 91.

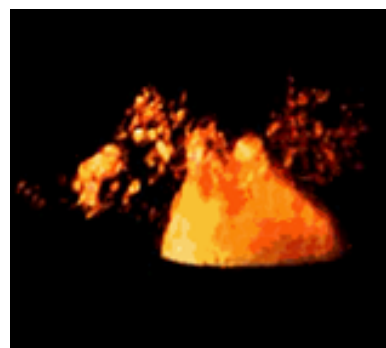
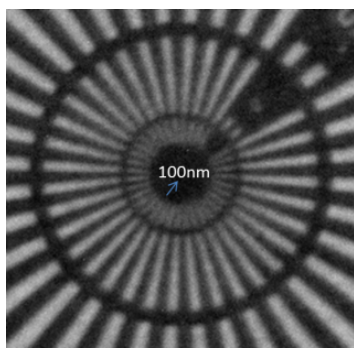


Figure 1. The TXM imaging of resolution target **Figure 2.** 3D imaging of particles based EST

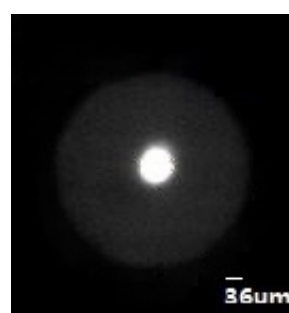
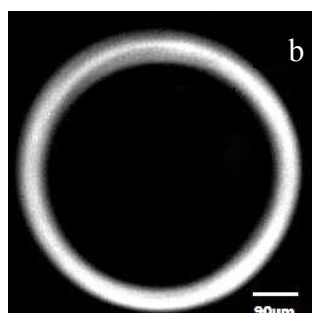


Figure 3. (a) The far-field pattern of the moncapillary; (b) The focused spot

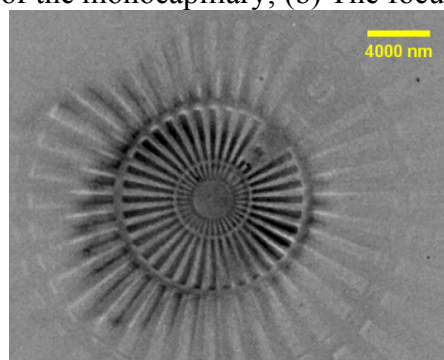


Figure 4. The TXM imaging of 100nm resolution target